



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

RECEIVED
By Tracy Crews at 8:35 am, Mar 10, 2020

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500225	NAME OF AGENCY Trenton Police Department	DATE OF INSPECTION 03/09/2020
------------------------	---	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 610 Main Street, Trenton, Missouri 64683	TIME OF INSPECTION 16:37:31
--	--------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>03/09/2020 16:37:34</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>45.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG931104</u>	EXP. DATE <u>11/07/2021</u>
---	-----------------------	-----------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____
--	--------------------	--------------------------

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.		
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE		
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE		
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE		

TEST 1: 0.099	TEST 2: 0.101	TEST 3: 0.101
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 2	.05-.09: 0	.10-.14: 1	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Monthly maintenance
Standard change- Replace expired dry gas

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME MATTHEW W PRESTON
---------------	--------------------------------------

TYPE II PERMIT NUMBER 280316	EXPIRATION DATE 11/07/2020	TELEPHONE NUMBER 660-359-2121
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
Southeast District Office
2875 James Blvd, Poplar Bluff, MO 63901

STANDARD CHANGE

Trenton Police Department
INTOX dmt: 500225

Date: 03/09/2020
Time: 16:33:57



OPERATOR NAME:
MATTHEW W PRESTON
PERMIT NUMBER: 280316
EXPIRATION DATE: 11/07/2020
MISC:
REPLACE EXPIRED DRYGAS TANK

LOT #: AG931104
SUPPLIER: INTOXIMETERS
EXPIRATION: 11/07/2021
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.096

BLANK TEST	0.000	16:34
INTERNAL STANDARD	VERIFIED	16:35
EXTERNAL STANDARD	0.097	16:35
BLANK TEST	0.000	16:36

Average = 0.0970
Std Dev = 0.0000
Spread = 0.0000

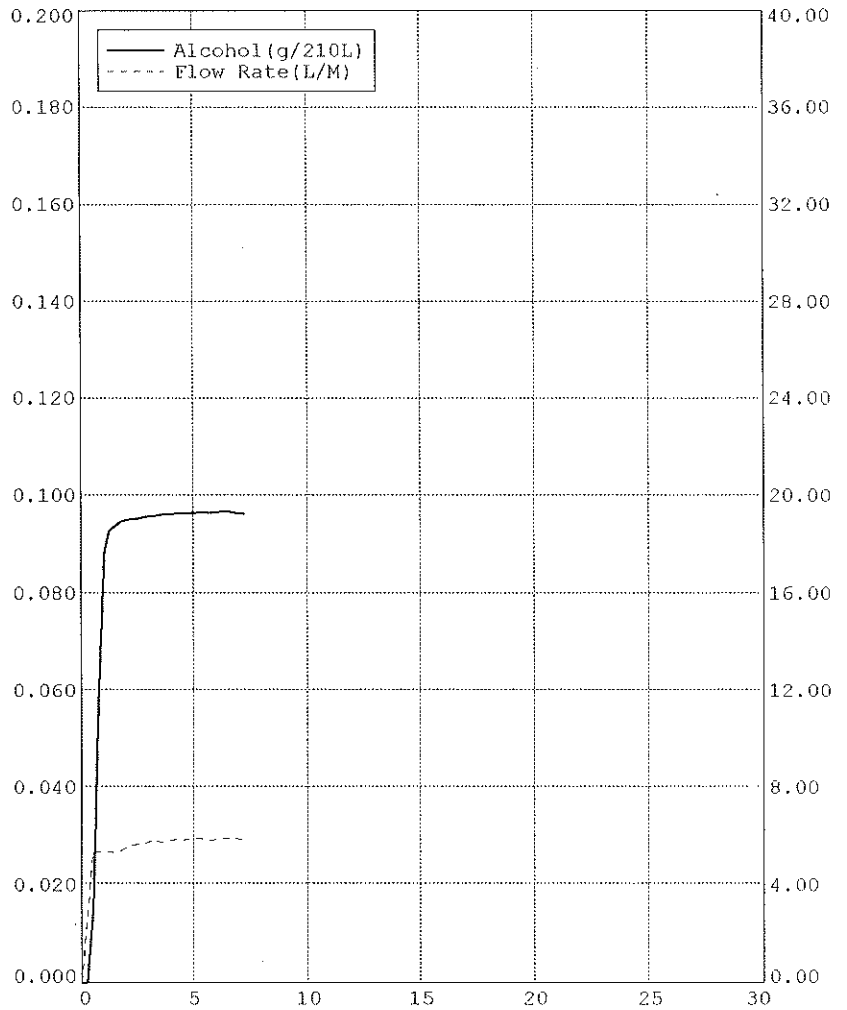



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



**PERMIT
 TYPE II**

MATTHEW W PRESTON

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 11/7/2018

NUMBER 280316

EXPIRES 11/7/2020

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 680-0771 (6-10)

LAB-4 (R6-10)



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator PRESTON, MATTHEW
 Permit No 280316
 Date Issued 11/7/2018 Date Expires 11/7/2020

