



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

RECEIVED
 By Tracy Crews at 8:17 am, Aug 24, 2020

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500266	NAME OF AGENCY UNIVERSITY OF MISSOURI POLICE DEPARTMENT	DATE OF INSPECTION 08/23/2020
LOCATION OF INSTRUMENT (STREET AND CITY) 901 VIRGINIA AVE, COLUMBIA		TIME OF INSPECTION 19:52:28

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>08/23/2020 19:52:30</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.8°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG019902 EXP. DATE 07/17/2022

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIM. SN _____ SIM. NIST EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.080 TEST 2: 0.080 TEST 3: 0.080


PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 1	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE  PRINT FULL NAME
JENNIFER PERRY

TYPE II PERMIT NUMBER
290031 EXPIRATION DATE
02/08/2021 TELEPHONE NUMBER
573-882-7201

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier

Intoximeters, Inc.

2081 Craig Road

St. Louis, Mo 63146

Test Date: 21-Jul-2020

Lot # AG019902 **Model** 108caccd

Exp. Date

17-Jul-2022

Cyl. Type

108

Component

Ethanol

Nitrogen

Certified Concentration

0.080 ± 0.002 BrAC (208 ppm)

Balance

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

RGM Serial No.

EB0010581

EB0010570

EB0010285

EB0010561

EB0010681

Concentration

392.1 ppm

259.8 ppm

208.0 ppm

103.6 ppm

52.12 ppm

RGM Serial No.

EB0010603

EB0010559

EB0010595

EB0010562

EB0010579

Concentration

393.0 ppm

258.2 ppm

208.3 ppm

104.2 ppm

52.81 ppm

CRM Serial No.

CC434668

CC234503

Concentration

800.0 ppm

253.0 ppm

CRM Serial No.

0056649

0056662

Concentration

390.1 ppm

150.2 ppm

Analytical Method:

NDIR

Digitally signed by Quality Control
Date: 2020.07.22 16:48:30 -05:00
Reason: Dry gas standard certification of analysis
Location: Airgas USA LLC (Lab)

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 3082.06

ISO 17034:2016 A2LA accredited. Certificate Number 3082.07



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 901 VIRGINIA AVE, COLUMBIA	INSTRUMENT SERIAL NUMBER 500266	DATE OF TEST 08/23/2020	TIME OBSERVATION PERIOD STARTED 19:00	TIME OF TEST 20:02:30
SUBJECT NAME TEST A TEST			DATE OF BIRTH 03/08/2000	
SUBJECT DRIVER'S LICENSE NUMBER NA			STATE NA	
ARRESTING OFFICER NA NA		ARRESTING OFFICER ID 14		
OPERATOR JENNIFER PERRY		OPERATOR PERMIT 290031	PERMIT EXP DATE 02/08/2021	
OBSERVER JENNIFER PERRY		OBSERVER PERMIT 290031	PERMIT EXP DATE	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JENNIFER PERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	20:03
INTERNAL STANDARD	VERIFIED	20:03
SUBJECT SAMPLE (Vol=1.76L)	0.000	20:03
BLANK TEST	0.000	20:04

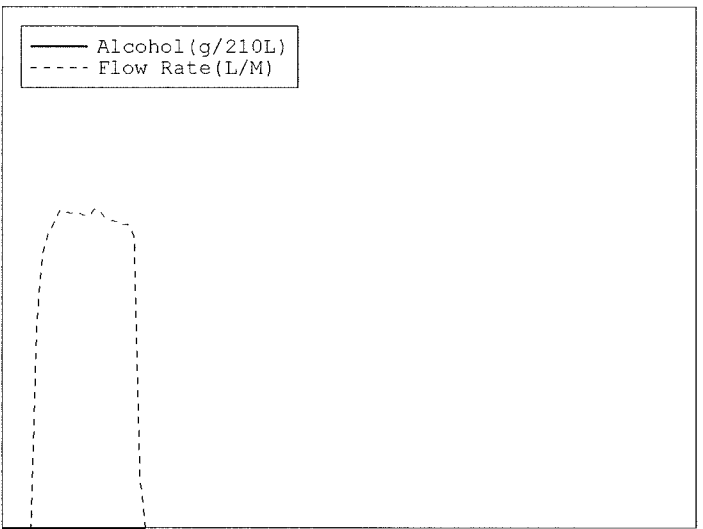

COMMENTS

CERTIFICATION BY OPERATOR BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.

SIGNATURE OF OPERATOR DATE
08/23/2020

WITNESS (IF ANY) DATE
08/23/2020



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
JENNIFER PERRY

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 2/8/2019

NUMBER 290031

EXPIRES 2/8/2021

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)

 **STATE OF MISSOURI**
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator PERRY, JENNIFER
 Permit No 290031
 Date Issued 2/8/2019 Date Expires 2/8/2021

