

RECEIVED

By Tracy Crews at 8:13 am, Jan 13, 2022



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500005	NAME OF AGENCY St. Louis County Police Department	DATE OF INSPECTION 12/15/2021
LOCATION OF INSTRUMENT (STREET AND CITY) 232 Vance Road, STL, MO 63088		TIME OF INSPECTION 08:28:08

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

 DIAGNOSTIC RECORD

DATE AND TIME <u>12/15/2021 08:28:11</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>46.5°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE
<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG013403</u> EXP. DATE <u>05/13/2022</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIM. SN _____ SIM. NIST EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

- 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.097	TEST 2: 0.097	TEST 3: 0.097
---------------	---------------	---------------

 PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

MSC Maintenance

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME RYAN A SCHILDKNECHT	
TYPE II PERMIT NUMBER 210253	EXPIRATION DATE 11/12/2023	TELEPHONE NUMBER 660-543-4573

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services
by mail, fax, or email



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500005	NAME OF AGENCY St. Louis County Police Department	DATE OF INSPECTION 12/15/2021
LOCATION OF INSTRUMENT (STREET AND CITY) 232 Vance Road, STL, MO 63088		TIME OF INSPECTION 08:28:08

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>12/15/2021 08:28:11</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>46.5°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE
---	--

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG013403</u>	EXP. DATE <u>05/13/2022</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C)	SIM. SN	SIM. NIST EXP DATE

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.097	TEST 2: 0.097	TEST 3: 0.097
---------------	---------------	---------------

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

MSC Maintenance

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME RYAN A SCHILDKNECHT	
TYPE II PERMIT NUMBER 210253	EXPIRATION DATE 11/12/2023	TELEPHONE NUMBER 660-543-4573

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services
 by mail, fax, or email



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 232 Vance Road, STL, MO 63088	INSTRUMENT SERIAL NUMBER 500005	DATE OF TEST 12/15/2021	TIME OBSERVATION PERIOD STARTED 08:05	TIME OF TEST 08:37:13
SUBJECT NAME TEST TEST			DATE OF BIRTH 12/05/2000	
SUBJECT DRIVER'S LICENSE NUMBER 1111111			STATE MO	
ARRESTING OFFICER TEST TEST		ARRESTING OFFICER ID 1		
OPERATOR RYAN A SCHILDKNECHT		OPERATOR PERMIT 210253	PERMIT EXP DATE 11/12/2023	
OBSERVER RYAN A SCHILDKNECHT		OBSERVER PERMIT 210253	PERMIT EXP DATE 11/12/2023	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by RYAN A SCHILDKNECHT. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	08:38
INTERNAL STANDARD	VERIFIED	08:38
SUBJECT SAMPLE (Vol=2.19L)	0.000	08:38
BLANK TEST	0.000	08:39

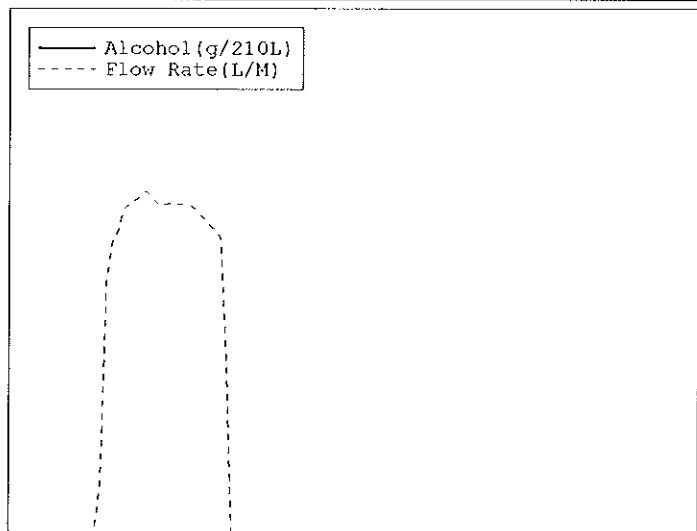


COMMENTS
MSC Test

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.

SIGNATURE OF OPERATOR  DATE
12/15/2021

WITNESS (IF ANY) DATE
12/15/2021



Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax: (314) 533-7328

Certificate of Analysis

Customer Name
 Exclusive Supplier
 Intoximeters, Inc.
 2081 Craig Road
 St. Louis, Mo 63146

Test Date: 18-May-2020

Lot # AG013403 Model 108cadd

<u>Exp. Date</u> 13-May-2022	<u>Cyl. Type</u> 108	<u>Component</u> Ethanol Nitrogen	<u>Certified Concentration</u> 0.100 ± 2% BrAC (260 ppm) Balance
--	--------------------------------	--	---

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

<u>RGM Serial No.</u>	<u>Concentration</u>	<u>RGM Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

<u>CRM Serial No.</u>	<u>Concentration</u>	<u>CRM Serial No.</u>	<u>Concentration</u>
CC434668	800.0 ppm	0056649	390.1 ppm
CC234503	253.0 ppm	0056662	150.2 ppm

Analytical Method: NDIR

Digitally signed by Quality Control
 Date: 2020.05.19 13:37:14 -05:00
 Reason: Dry gas standard certification of analysis
 Location: Airgas USA LLC (Lab)

Approved for Release: *Rod Marsala*
 Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 3082.06
 ISO 17034:2016 A2LA accredited. Certificate Number 3082.07



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

2

PERMIT
TYPE II
RYAN SCHILDKNECHT

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT, INTOXILYZER 8000, INTOX EC/IR II, ASIV W/PRINTER

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 11/12/2021

NUMBER 210253

EXPIRES 11/12/2023

MO 580-0771 (6-10)

Laura P. Day

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

Donald A. Ramsey

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (R6-10)



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.



Operator SCHILDKNECHT, RYAN
Permit No 210253
Date Issued 11/12/2021 Date Expires 11/12/2023