



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

| | | |
|-------------------------------|---|---|
| INTOX DMT SN 500016 | NAME OF AGENCY Higginsville Police Department | DATE OF INSPECTION 03/22/2021 |
|-------------------------------|---|---|

| | |
|---|---------------------------------------|
| LOCATION OF INSTRUMENT (STREET AND CITY) 12 W 19th Street, Higginsville, MO | TIME OF INSPECTION 16:12:23 |
|---|---------------------------------------|

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

| | |
|--|---|
| <input checked="" type="checkbox"/> DIAGNOSTIC RECORD | |
| DATE AND TIME <u>03/22/2021 16:12:25</u> | <input checked="" type="checkbox"/> DETECTOR |
| <input checked="" type="checkbox"/> PROGRAM | <input checked="" type="checkbox"/> FILTER 1 |
| <input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u> | <input checked="" type="checkbox"/> FILTER 2 |
| <input checked="" type="checkbox"/> BREATH TUBE <u>44.9°C</u> | <input checked="" type="checkbox"/> FILTER 3 |
| <input checked="" type="checkbox"/> PUMP | <input checked="" type="checkbox"/> INTERNAL STANDARD |

| | |
|---|--|
| BREATH ANALYZER ACCURACY STANDARDS | |
| <input type="checkbox"/> SIMULATOR STANDARD | <input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE |

| | | |
|---|-----------------------|-----------------------------|
| <input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u> | LOT # <u>AG031504</u> | EXP. DATE <u>11/10/2022</u> |
|---|-----------------------|-----------------------------|

| | | |
|--|---------------|--------------------------|
| <input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____ | SIM. SN _____ | SIM. NIST EXP DATE _____ |
|--|---------------|--------------------------|

| |
|--|
| <input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used. |
| <input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE |
| <input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE |
| <input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE |

| | | |
|---------------|---------------|---------------|
| TEST 1: 0.101 | TEST 2: 0.100 | TEST 3: 0.100 |
|---------------|---------------|---------------|

| |
|--|
| <input checked="" type="checkbox"/> PERFORM R.F.I. TEST |
|--|

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

| | | | | | |
|-------------|----------|------------|------------|------------|-------------|
| REFUSALS: 0 | 0-.04: 4 | .05-.09: 2 | .10-.14: 0 | .15-.19: 0 | OVER .19: 1 |
|-------------|----------|------------|------------|------------|-------------|

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

| | |
|---------------|--|
| SIGNATURE | PRINT FULL NAME QUINTON L DINOVI |
|---------------|--|

| | | |
|--|--------------------------------------|---|
| TYPE II PERMIT NUMBER 290226 | EXPIRATION DATE 10/01/2021 | TELEPHONE NUMBER 660-584-2104 |
|--|--------------------------------------|---|

RETURN COMPLETED REPORT TO THE **Breath Alcohol Program, Missouri Department of Health and Senior Services**
by mail, fax, or email

STANDARD CHANGE

Higginsville Police Department
INTOX dmt: 500016

Date: 03/22/2021
Time: 16:08:46


OPERATOR NAME:
QUINTON L DINOVI
PERMIT NUMBER: 290226
EXPIRATION DATE: 10/01/2021

LOT #: AG031504
SUPPLIER: INTOXIMETERS
EXPIRATION: 11/10/2022
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.096

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 16:09 |
| INTERNAL STANDARD | VERIFIED | 16:09 |
| EXTERNAL STANDARD | 0.097 | 16:10 |
| BLANK TEST | 0.000 | 16:10 |

Average = 0.0970
Std Dev = 0.0000
Spread = 0.0000

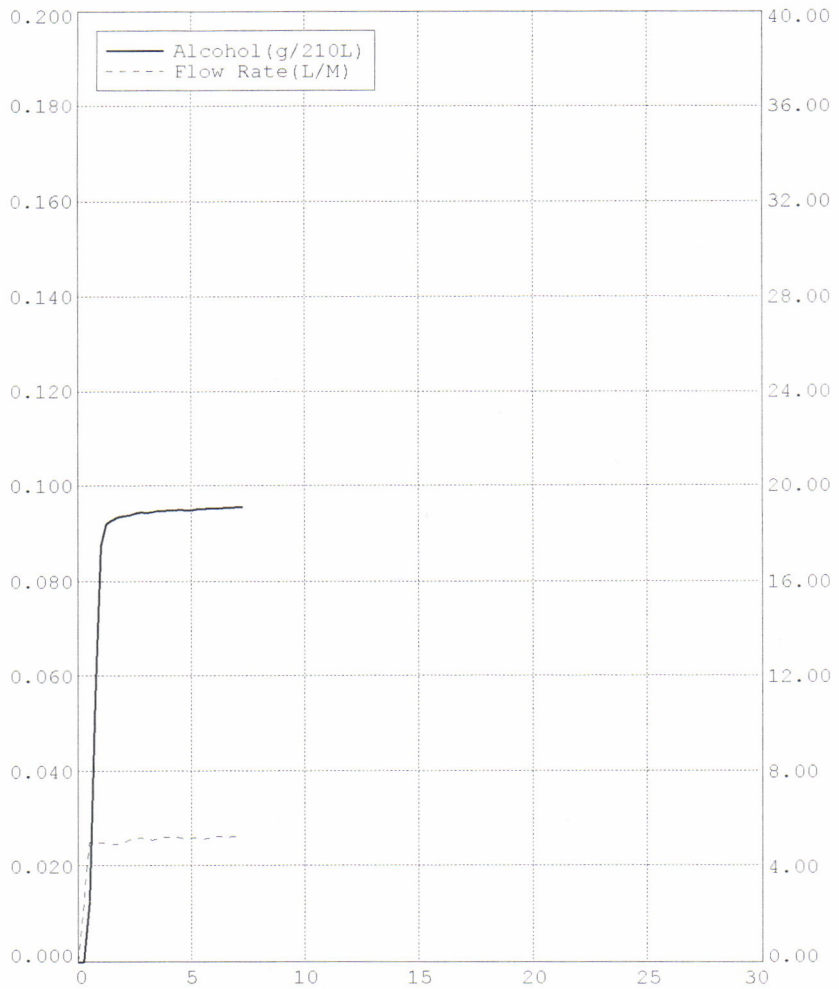



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
QUINTON L. DiNOVI

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 10/1/2019

NUMBER 290226

EXPIRES 10/1/2021

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)

STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator **DINOVI, QUINTON**
 Permit No **290226**
 Date issued **10/1/2019** Date Expires **10/1/2021**