



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

RECEIVED

By Tracy Crews at 3:37 pm, Feb 05, 2021

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500045	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 02/04/2021
LOCATION OF INSTRUMENT (STREET AND CITY) Pettis Co Jail, 333 S Lamine, Sedalia, MO 65301		TIME OF INSPECTION 09:27:52

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>02/04/2021 09:27:54</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>46.0°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG905203 EXP. DATE 02/21/2021

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIM. SN _____ SIM. NIST EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.099	TEST 2: 0.098	TEST 3: 0.098
----------------------	----------------------	----------------------

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 1	.10-.14: 3	.15-.19: 2	OVER .19: 2
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Time Sync to 848 HP MCD

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JERRY W HUNTER	
TYPE II PERMIT NUMBER 200227	EXPIRATION DATE 08/18/2022	TELEPHONE NUMBER 816-622-0800

RETURN COMPLETED REPORT TO THE **Breath Alcohol Program, Missouri Department of Health and Senior Services**
by mail, fax, or email

Airgas.

Airgas USA LLC (LAB)
3500 Bernard Street
St. Louis, Mo. 63103
Ph: (314) 533-3100
Fax: (314) 533-7328

Certificate of Analysis

Customer Name
Exclusive Supplier
Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 22-Feb-2019

Lot # AG905203 Model 108cadd

Exp. Date
21-Feb-2021

Cyl. Type
108

Component
Ethanol
Nitrogen

Certified Concentration
0.100 ± 2% BrAC (260 ppm)
Balance

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

<u>RGM Serial No.</u>	<u>Concentration</u>
EB0010561	392.1 ppm
EB0010570	259.8 ppm
EB0010285	208.0 ppm
EB0010561	103.6 ppm
EB0010681	52.12 ppm

<u>RGM Serial No.</u>	<u>Concentration</u>
EB0010603	393.0 ppm
EB0010559	258.2 ppm
EB0010595	208.3 ppm
EB0010562	104.2 ppm
EB0010579	52.81 ppm

<u>CRM Serial No.</u>	<u>Concentration</u>
CC434668	800.0 ppm
CC234503	253.0 ppm

<u>CRM Serial No.</u>	<u>Concentration</u>
0056649	390.1 ppm
0056662	150.2 ppm

Analytical Method: NDIR

Digitally signed by Quality Control
Date: 2019.02.27 13:07:54 -08:00
Reason: Dry gas standard certification of analysis
Location: Airgas USA, LLC (Lab)

Approved for Release:


Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 3082.06
ISO 17034:2016 A2LA accredited. Certificate Number 3082.07

STANDARD CHANGE

Missouri State Highway Patrol
INTOX dmt: 500045

Date: 02/04/2021
Time: 09:42:23


OPERATOR NAME:
JERRY W HUNTER
PERMIT NUMBER: 200227
EXPIRATION DATE: 08/18/2022

LOT #: AG024403
SUPPLIER: INTOXIMETERS
EXPIRATION: 08/31/2022
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.095

BLANK TEST	0.000	09:43
INTERNAL STANDARD	VERIFIED	09:43
EXTERNAL STANDARD	0.095	09:43
BLANK TEST	0.000	09:44

Average = 0.0950
Std Dev = 0.0000
Spread = 0.0000

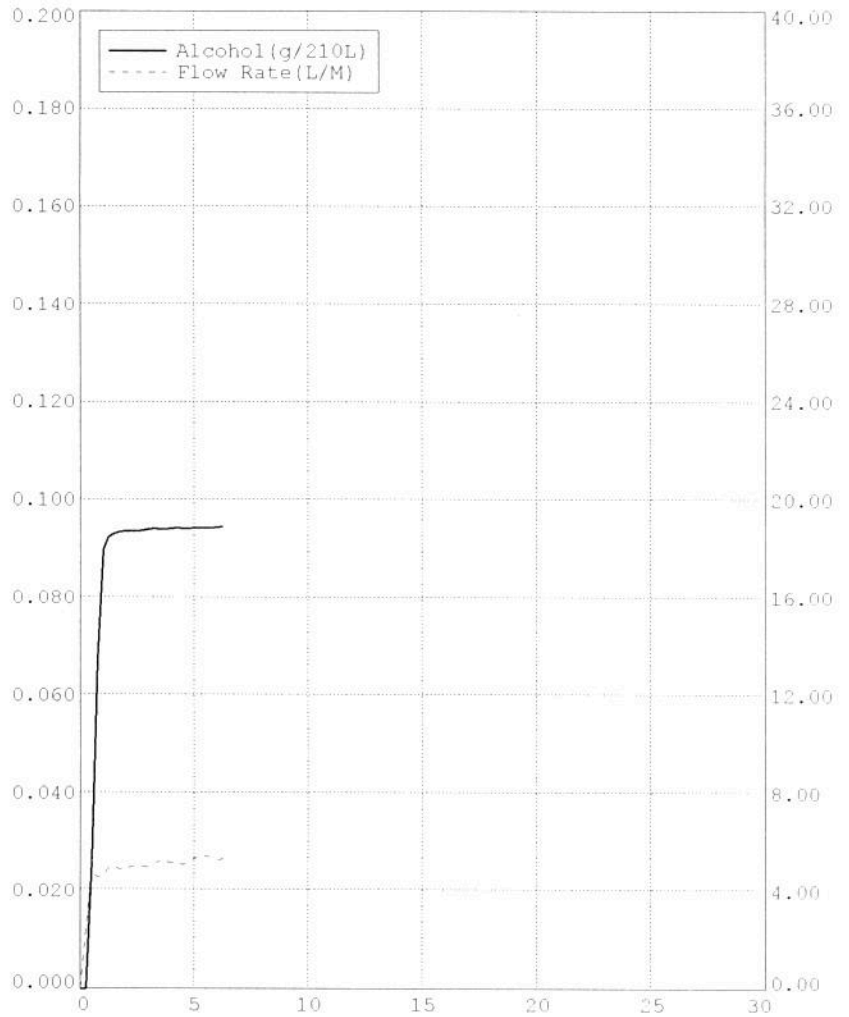

Jerry W Hunter
#818



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

2

PERMIT
TYPE II
JERRY W. HUNTER

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 8/18/2020
 NUMBER 200227
 EXPIRES 8/18/2022

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.



Operator HUNTER, JERRY
 Permit No 200227
 Date Issued 8/18/2020 Date Expires 8/18/2022