

RECEIVED

By Tracy Crews at 8:30 am, Nov 12, 2021



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500252	NAME OF AGENCY Cameron Police Department	DATE OF INSPECTION 11/08/2021
------------------------	---	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 101 North Chestnut, Cameron, Missouri 64429	TIME OF INSPECTION 03:32:01
---	--------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>11/08/2021 03:32:03</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.8°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG931603</u>	EXP. DATE <u>11/12/2021</u>
---	-----------------------	-----------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIM. SN _____	SIM. NIST EXP DATE _____
--	---------------	--------------------------

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.
<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: <u>0.078</u>	TEST 2: <u>0.079</u>	TEST 3: <u>0.079</u>
----------------------	----------------------	----------------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: <u>2</u>	0-.04: <u>1</u>	.05-.09: <u>0</u>	.10-.14: <u>1</u>	.15-.19: <u>1</u>	OVER .19: <u>1</u>
--------------------	-----------------	-------------------	-------------------	-------------------	--------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JAMES C PROCTOR
--	------------------------------------

TYPE II PERMIT NUMBER 210046	EXPIRATION DATE 03/16/2023	TELEPHONE NUMBER 816-632-6521
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services
by mail, fax, or email



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 101 North Chestnut, Cameron, Missouri	INSTRUMENT SERIAL NUMBER 500252	DATE OF TEST 11/08/2021	TIME OBSERVATION PERIOD STARTED 03:16	TIME OF TEST 03:40:55
SUBJECT NAME MONTHLY TEST			DATE OF BIRTH 11/08/2000	
SUBJECT DRIVER'S LICENSE NUMBER MO112021			STATE MO	
ARRESTING OFFICER JAMES C PROCTOR		ARRESTING OFFICER ID 107		
OPERATOR JAMES C PROCTOR		OPERATOR PERMIT 210046	PERMIT EXP DATE 03/16/2023	
OBSERVER JAMES C PROCTOR		OBSERVER PERMIT 210046	PERMIT EXP DATE 03/16/2023	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JAMES C PROCTOR. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	03:41
INTERNAL STANDARD	VERIFIED	03:42
SUBJECT SAMPLE (Vol=3.01L)	0.000	03:42
BLANK TEST	0.000	03:43

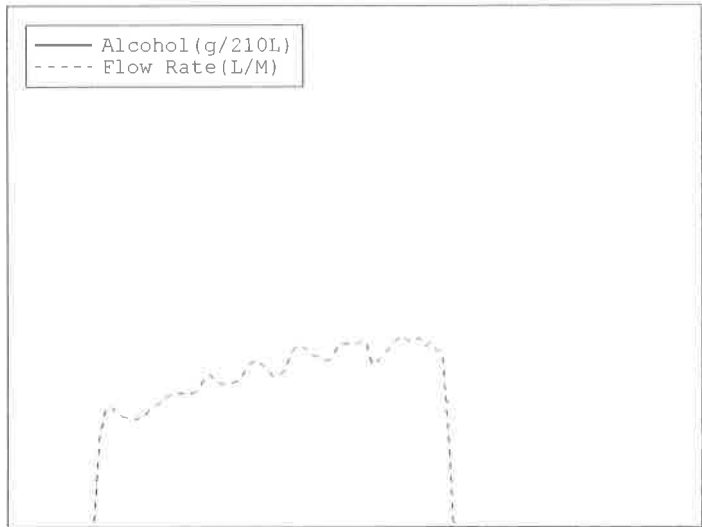


COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.

SIGNATURE OF OPERATOR 	DATE 11/08/2021
WITNESS (IF ANY)	DATE 11/08/2021



Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax: (314) 533-7328

Certificate of Analysis

Test Date: 12-Nov-2019

Customer Name
 Exclusive Supplier
 Intoximeters, Inc.
 2081 Craig Road
 St. Louis, Mo 63146

Lot # AG931603 Model 108cccd

<u>Exp. Date</u> 12-Nov-2021	<u>Cyl. Type</u> 108	<u>Component</u> Ethanol Nitrogen	<u>Certified Concentration</u> 0.080 ± 0.002 BrAC (208 ppm) Balance
---------------------------------	-------------------------	---	---

Certification Traceable to NLS.T. RGM and to CRM Ethanol Standards:

<u>RGM Serial No.</u>	<u>Concentration</u>	<u>RGM Serial No.</u>	<u>Concentration</u>
EB001 0581	392.1 ppm	EB001 0603	393.0 ppm
EB001 0570	259.8 ppm	EB001 0559	258.2 ppm
EB001 0285	208.0 ppm	EB001 0595	208.3 ppm
EB001 0561	103.6 ppm	EB001 0562	104.2 ppm
EB001 0681	52.12 ppm	EB001 0579	52.81 ppm

<u>CRM Serial No.</u>	<u>Concentration</u>	<u>CRM Serial No.</u>	<u>Concentration</u>
CC434668	800.0 ppm	0056649	390.1 ppm
CC234503	253.0 ppm	0056662	150.2 ppm

Analytical Method: NDIR

Digitally signed by Quality Control
 Date: 2019.11.13 10:21:47 -0500
 Reason: Dry gas standard certification of analysis
 Location: Airgas USA LLC (Lab)

Approved for Release: Rod Marsala
 Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 3082.06
 ISO 17034:2016 A2LA accredited. Certificate Number 3082.07



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
JAMES C. PROCTOR

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 3/16/2021

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

NUMBER 210046

EXPIRES 3/16/2023

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 80-077 (5-10)

LAB-4 (PG-10)

STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named individual is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator: **PROCTOR, JAMES**
Permit No: **210046**
Date Issued: **3/16/2021** Date Expires: **3/16/2023**