



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM

INTOX EC/IR II MAINTENANCE REPORT

REPORT #3

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days). Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service. Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX EC/IR II SN 12822	NAME OF AGENCY Harrisonville Police	DATE OF INSPECTION 12/14/2022
----------------------------	--	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 205 N. Lexington Harrisonville	TIME OF INSPECTION 03:24 CST
--	---------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
<input checked="" type="checkbox"/> BLANK CHECK	<input checked="" type="checkbox"/> CO2 CHECK
<input checked="" type="checkbox"/> FC 1 TEMP	<input checked="" type="checkbox"/> FLOW CHECK
<input checked="" type="checkbox"/> SRC TEMP	<input checked="" type="checkbox"/> FCB CHECK
<input checked="" type="checkbox"/> DET TEMP	<input checked="" type="checkbox"/> CRC COMP CHECK
<input checked="" type="checkbox"/> BT TEMP	<input checked="" type="checkbox"/> CRC CAL CHECK
<input checked="" type="checkbox"/> STD 2 TEMP	<input checked="" type="checkbox"/> PRINT TEST
<input checked="" type="checkbox"/> ETH CHECK	

BREATH ANALYZER ACCURACY STANDARDS		
<input type="checkbox"/> SIMULATOR SOLUTION	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE	
<input checked="" type="checkbox"/> STANDARD SUPPLIER Intoximeters	LOT# AG106801	EXP. DATE 03/09/2023
<input type="checkbox"/> SIMULATOR TEMP (34°C ±0.2°C)	SIM. SN	SIM. NIST EXP DATE

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard solution. All three tests must be within +5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used.
<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 0.078 g/210L	TEST 2 0.078 g/210L	TEST 3 0.078 g/210L
---------------------	---------------------	---------------------

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS 0	0-.04 0	.05-.09 0	.10-.14 2	.15-.19 0	OVER .19 2
------------	---------	-----------	-----------	-----------	------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

N/A

INSPECTING OFFICER		
SIGNATURE 	PRINT FULL NAME R. STARK	
TYPE 11 PERMIT NUMBER 210168	EXPIRATION DATE 08/04/2023	TELEPHONE NUMBER (816) 380-8940

RETURN COMPLETED REPORT TO THE:
 Breath Alcohol Program, Missouri Department of Health and Senior Services,
 by mail, fax, or e-mail



Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax: (314) 533-7328

Certificate of Analysis

Customer Name
 Exclusive Supplier
 Intoximeters, Inc.
 2081 Craig Road
 St. Louis, Mo 63146

Test Date: 9-Mar-2021

Lot # AG106801 Model 108cadd

<u>Exp. Date</u> 9-Mar-2023	<u>Cyl. Type</u> 108	<u>Component</u> Ethanol Nitrogen	<u>Certified Concentration</u> 0.080 ± 0.002 BrAC (218 ppm) Balance
--------------------------------	-------------------------	---	---

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

<u>RGM Serial No.</u>	<u>Concentration</u>	<u>RGM Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm
<u>CRM Serial No.</u>	<u>Concentration</u>	<u>CRM Serial No.</u>	<u>Concentration</u>
CC727481	800.0 ppm	CC727493	390.0 ppm
CC727496	253.0 ppm	CC727498	150.0 ppm

Analytical Method: NDIR

Approved for Release: _____



ISO 17025:2005 A2LA accredited. Certificate Number 3082.06
 ISO 17034:2016 A2LA accredited. Certificate Number 3082.07

University of Central Missouri

Missouri Safety Center - Institute for Public Safety

awards
RYAN A. STARK

Certificate of Completion for 8.0 hours of instruction in

TYPE - II LAB INTOX EC/IR II

The POST approved program for:

<u>3.0</u>	<u>Technical Studies</u>
No. of CEH's	Core Curriculum Area
<u>5.0</u>	<u>Skill Development</u>
No. of CEH's	Core Curriculum Area
<u>0.0</u>	<u>Interpersonal Perspectives</u>
No. of CEH's	Core Curriculum Area
<u>0.0</u>	<u>Legal Studies</u>
No. of CEH's	Core Curriculum Area

Joanne Kurt-Hilditch, Ph.D.


Senior Director

Matthew Bond

Program Manager

MISSOURI

Safety Center

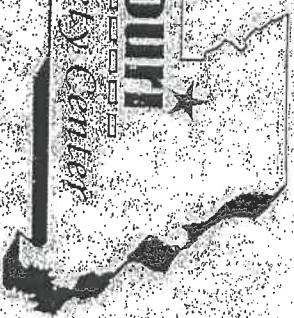

A Missouri Post

"Approved Provider"

Given in

Warrensburg, Missouri

on July 26, 2021

HARRISONVILLE POLICE DEPT.



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II

RYAN STARK

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

ALCO-SENSOR IV WITH PRINTER

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE: 8/4/2021
 NUMBER: 210168
 EXPIRES: 8/4/2023
 C: 580:0771 (6-10)

Laura A. Way
 DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

[Signature]
 DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES
 LAB 4 (R6-10)

STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator: STARK, RYAN
 Permit No: 210168
 Date Issued: 8/4/2021 Date Expires: 8/4/2023