

RECEIVED

By Tracy Crews at 8:55 am, Jul 22, 2022



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500023	NAME OF AGENCY Caruthersville Police Department	DATE OF INSPECTION 07/21/2022
LOCATION OF INSTRUMENT (STREET AND CITY) 1400 Ward Ave. Caruthersville, MO.		TIME OF INSPECTION 12:35:32

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>07/21/2022 12:35:33</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG211003</u>	EXP. DATE <u>04/20/2024</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C)	SIM. SN	SIM. NIST EXP DATE

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.	
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE	
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE	
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE	

TEST 1: 0.098	TEST 2: 0.098	TEST 3: 0.098
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST
---

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:					
REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

INSPECTING OFFICER		
SIGNATURE 	PRINT FULL NAME TERRY W PRIVETT	
TYPE II PERMIT NUMBER 210329	EXPIRATION DATE 12/30/2023	TELEPHONE NUMBER 573-333-0216

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email



Airgas USA LLC (LAB)  
3500 Bernard Street  
St. Louis, Mo. 63103  
Ph: (314) 533-3100  
Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**  
*Exclusive Supplier*  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

**Test Date:** 21-Apr-2022

**Lot #** AG211003 **Model** 108

<b>Exp Date</b>	<b>Cyl. Type</b>	<b>Component</b>	<b>Certified Concentration</b>
20-Apr-2024	108	Ethanol Nitrogen	0.100 ± 2% BrAC (260 ppm)

**Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:**

<b>RGM Serial No.</b>	<b>Concentration</b>	<b>RGM Serial No.</b>	<b>Concentration</b>
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010562	104.2 ppm
EB0010561	103.7 ppm	EB0010579	52.94 ppm
EB0010681	52.22 ppm		

<b>CRM Serial No.</b>	<b>Concentration</b>	<b>CRM Serial No.</b>	<b>Concentration</b>
CC727481	800.0 ppm	CC727493	390.0 ppm
CC727496	253.0 ppm	CC727498	150.0 ppm

**Analytical Method:** NDIR

Approved for Release: \_\_\_\_\_

Rod Marsala

**ISO 17025:2017 A2LA accredited. Certificate Number 3082.06**  
**ISO 17034:2016 A2LA accredited. Certificate Number 3082.07**

STANDARD CHANGE

-----  
Caruthersville Police Department  
INTOX dmt: 500023  
-----

Date: 07/21/2022  
Time: 12:31:46


OPERATOR NAME:  
TERRY W PRIVETT  
PERMIT NUMBER: 210329  
EXPIRATION DATE: 12/30/2023

LOT #: AG211003  
SUPPLIER: INTOXIMETERS  
EXPIRATION: 04/20/2024  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.100  
TARGET: 0.099

BLANK TEST	0.000	12:32
INTERNAL STANDARD	VERIFIED	12:32
EXTERNAL STANDARD	0.098	12:33
BLANK TEST	0.000	12:34

Average = 0.0980  
Std Dev = 0.0000  
Spread = 0.0000

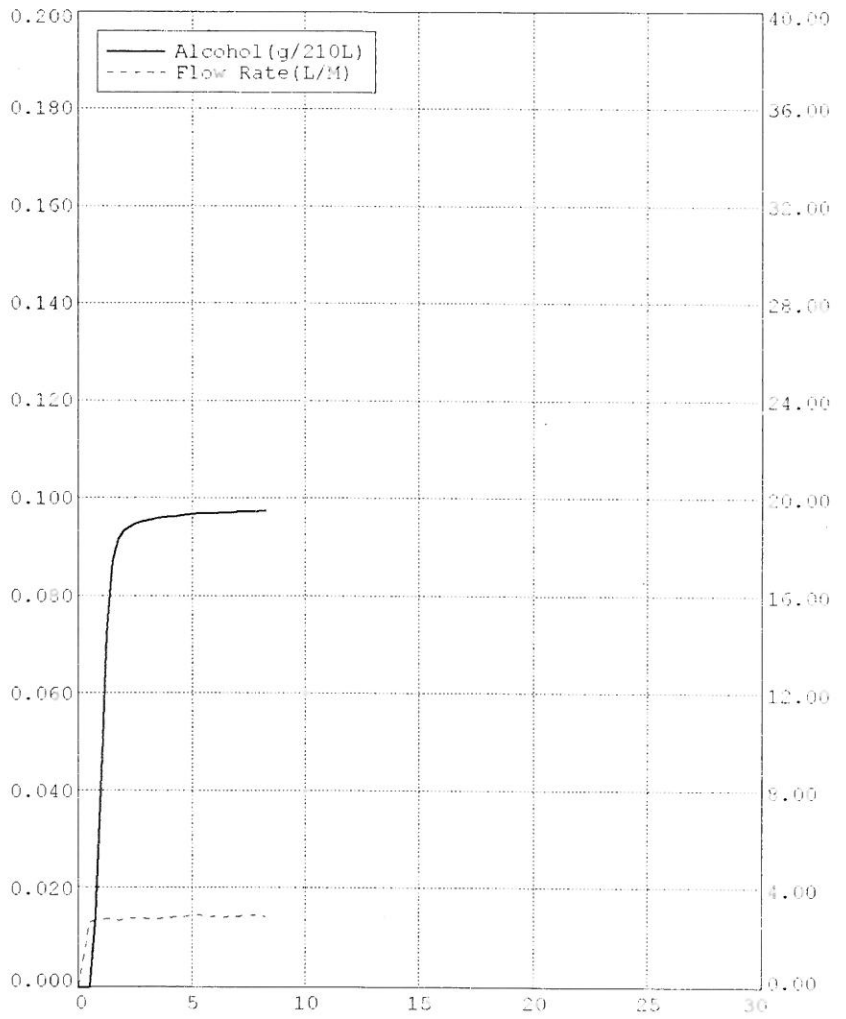

JK



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM



**PERMIT**  
**TYPE II**  
**TERRY W. PRIVETT**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE **12/30/2021**

NUMBER **210329**

EXPIRES **12/30/2023**

*Laura Q. Day*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*Donald A. Ramsey*

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES



**STATE OF MISSOURI**  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*

**Operator** PRIVETT, TERRY  
**Permit No** 210329  
**Date Issued** 12/30/2021    **Date Expires** 12/30/2023

