

**RECEIVED**

By Tracy Crews at 1:56 pm, Oct 19, 2022



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500225	NAME OF AGENCY Trenton Police Department	DATE OF INSPECTION 10/10/2022
LOCATION OF INSTRUMENT (STREET AND CITY) 610 Main Street, Trenton, Missouri 64683		TIME OF INSPECTION 08:49:24

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>10/10/2022 08:49:27</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>45.5°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG130104</u>	EXP. DATE <u>10/28/2023</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIM. SN _____	SIM. NIST EXP DATE _____

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.	
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE	
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE	
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE	

TEST 1: 0.104	TEST 2: 0.104	TEST 3: 0.104
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST
---

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

MSC TEST

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME RYAN SCHILDKNECHT
---------------	--------------------------------------

TYPE II PERMIT NUMBER 210253	EXPIRATION DATE 11/12/2023	TELEPHONE NUMBER 660-543-4573
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services  
by mail, fax, or email



**Airgas USA LLC (LAB)**  
 3500 Bernard Street  
 St. Louis, Mo. 63103  
 Ph: (314) 533-3100  
 Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**  
*Exclusive Supplier*  
 Intoximeters, Inc.  
 2081 Craig Road  
 St. Louis, Mo 63146

**Test Date:** 1-Nov-2021

**Lot # AG130104 Model 108**

<b>Exp Date</b> 28-Oct-2023	<b>Cyl. Type</b> 108	<b>Component</b> Ethanol Nitrogen	<b>Certified Concentration</b> 0.100 ± 2% BrAC (260 ppm)
--------------------------------	-------------------------	---	---

**Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:**

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CC434668	800.0 ppm	0056649	390.1 ppm
CC234503	253.0 ppm	0056662	150.2 ppm

**Analytical Method:** NDIR

Digitally signed by: Quality Control  
 Reason: Dry gas standard certification of analysis  
 Location: Airgas USA LLC (Lab)  
 Date: 11.05.2021 11:46

**Approved for Release:** \_\_\_\_\_  
  
 Rod Marsala

**ISO 17025:2017 A2LA accredited. Certificate Number 3082.06**  
**ISO 17034:2016 A2LA accredited. Certificate Number 3082.07**

DIAGNOSTIC RECORD

-----  
Trenton Police Department  
INTOX dmt: 500225  
-----

Date: 10/10/2022  
Time: 08:57:19

VERSIONS  
Missouri DHSS Version: 1.00  
PIC: 3.03  
Questions: 2.7

TEMPERATURES

Sample Chamber = 48.7°C	PASSED
Breath Tube = 45.0°C	PASSED
Simulator Hose = 45.0°C	PASSED

PUMP INFO  
Flow Rate = 5.260 L/M PASSED

DETECTOR INFO  
PUMP ON PASSED  
PUMP OFF PASSED

FILTER INFO  
Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD  
Xq = 0.099 1.52% PASSED



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
**BLOOD ALCOHOL TEST REPORT - INTOX DMT**

FORM #11


LOCATION OF INSTRUMENT 610 Main Street, Trenton, Missouri 64683	INSTRUMENT SERIAL NUMBER 500225	DATE OF TEST 10/10/2022	TIME OBSERVATION PERIOD STARTED 13:00	TIME OF TEST 13:40:32
SUBJECT NAME TEST TEST			DATE OF BIRTH 12/12/2000	
SUBJECT DRIVER'S LICENSE NUMBER 1			STATE MO	
ARRESTING OFFICER TEST TEST		ARRESTING OFFICER ID 1		
OPERATOR RYAN SCHILDKNECHT		OPERATOR PERMIT 210253	PERMIT EXP DATE 11/12/2023	
OBSERVER RYAN SCHILDKNECHT		OBSERVER PERMIT 210253	PERMIT EXP DATE 11/12/2023	

**OPERATIONAL CHECKLIST: INTOX DMT**

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by RYAN SCHILDKNECHT. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

**SUBJECT TEST RESULTS**

BLANK TEST	0.000	13:41
INTERNAL STANDARD	VERIFIED	13:41
SUBJECT SAMPLE (Vol=1.68L)	0.000	13:41
BLANK TEST	0.000	13:42

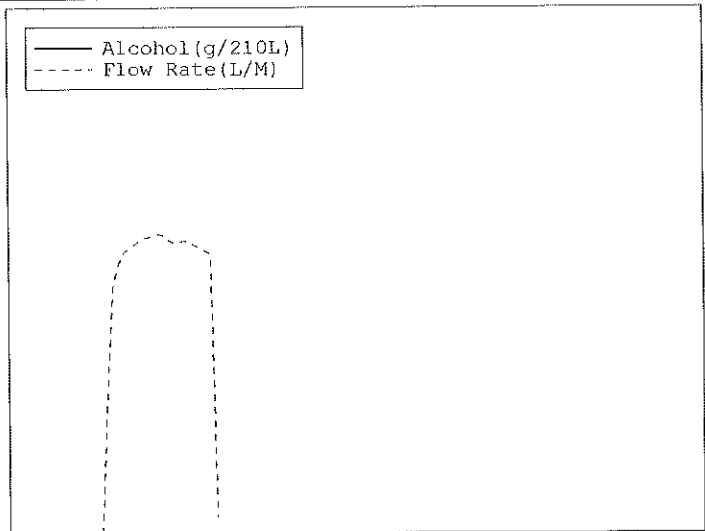

COMMENTS  
 msc test

**CERTIFICATION BY OPERATOR**

BAC  
 0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.

SIGNATURE OF OPERATOR 	DATE 10/10/2022
WITNESS (IF ANY)	DATE 10/10/2022



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

2

**PERMIT**  
**TYPE II**  
**RYAN SCHILDKNECHT**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT, INTOXILYZER 8000, INTOX EC/IR II, ASIV W/PRINTER**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 11/12/2021

NUMBER 210253

EXPIRES 11/12/2023

*Laura Q. Nay*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*Donald B. Kauffman*

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (R6-10)

MO 580-0771 (6-10)

STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*



Operator SCHILDKNECHT, RYAN  
 Permit No 210253  
 Date issued 11/12/2021 Date Expires 11/12/2023