

RECEIVED

By Tracy Crews at 7:54 am, Apr 14, 2022



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500252	NAME OF AGENCY Cameron Police Department	DATE OF INSPECTION 04/08/2022
LOCATION OF INSTRUMENT (STREET AND CITY) 101 North Chestnut, Cameron, Missouri 64429		TIME OF INSPECTION 02:59:01

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>04/08/2022 02:59:04</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>46.9°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG129201</u>	EXP. DATE <u>10/19/2023</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C)	SIM. SN	SIM. NIST EXP DATE

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.
<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: <u>0.079</u>	TEST 2: <u>0.079</u>	TEST 3: <u>0.079</u>
----------------------	----------------------	----------------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:					
REFUSALS: 0	0-.04: 1	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 1

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER	
SIGNATURE 	PRINT FULL NAME JAMES C PROCTOR
TYPE II PERMIT NUMBER 2100046	TELEPHONE NUMBER 816-632-6521
EXPIRATION DATE 03/16/2023	

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email



Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax (314) 533-7328

Certificate of Analysis

Customer Name
 Exclusive Supplier
 Intoximeters, Inc.
 2081 Craig Road
 St. Louis, Mo 63146

Test Date: 20-Oct-2021

Lot # AG129201 Model 108

Exp Date	Cyl. Type	Component	Certified Concentration
19-Oct-2023	108	Ethanol Nitrogen	0.080 ± 0.002 BrAC (208 ppm)

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CC434668	800.0 ppm	0056649	390.1 ppm
CC234503	253.0 ppm	0056662	150.2 ppm

Analytical Method: NDIR

Digitally signed by:Quality Control
 Reason:Dry gas standard certification of analysis
 Location:Airgas USA,LLC (Lab)
 Date:10.20.2021 17:16

Approved for Release: 
 Rod Marsala

ISO 17025:2017 A2LA accredited. Certificate Number 3082.06
 ISO 17034:2016 A2LA accredited. Certificate Number 3082.07

STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

2

PERMIT
TYPE II

JAMES C. PROCTOR

INTOX DMT

2767073

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

2767066

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

2767073


MISSOURI

STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

This permit certifies that the operator is competent to operate any certified breath alcohol instrument used for the determination of the alcohol content in breath form of subjects in Missouri.

Operator: PROCTOR, JAMES
Permit No: 27066
Date Issued: 1/15/2011 The State of Missouri





MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 101 North Chestnut, Cameron, Missouri	INSTRUMENT SERIAL NUMBER 500252	DATE OF TEST 04/08/2022	TIME OBSERVATION PERIOD STARTED 02:40	TIME OF TEST 03:08:18
SUBJECT NAME MONTHLY TEST			DATE OF BIRTH 09/05/1998	
SUBJECT DRIVER'S LICENSE NUMBER 04082022			STATE MO	
ARRESTING OFFICER JAMES C PROCTOR		ARRESTING OFFICER ID 107		
OPERATOR JAMES C PROCTOR		OPERATOR PERMIT 2100046	PERMIT EXP DATE 03/16/2023	
OBSERVER JAMES C PROCTOR		OBSERVER PERMIT 2100046	PERMIT EXP DATE 03/16/2023	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JAMES C PROCTOR. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	03:09
INTERNAL STANDARD	VERIFIED	03:09
SUBJECT SAMPLE (Vol=3.44L)	0.000	03:09
BLANK TEST	0.000	03:10

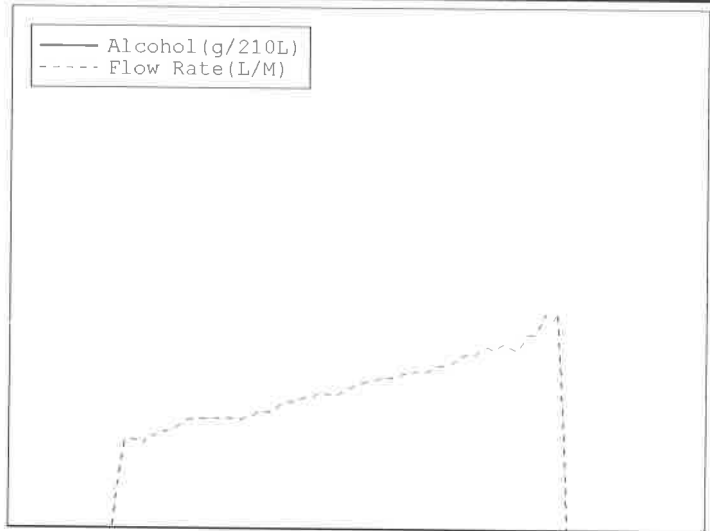

COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.

SIGNATURE OF OPERATOR 	DATE 04/08/2022
WITNESS (IF ANY)	DATE 04/08/2022