

RECEIVED

By Tracy Crews at 8:50 am, Jun 13, 2022



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500281	NAME OF AGENCY St Robert Police Department	DATE OF INSPECTION 06/11/2022
LOCATION OF INSTRUMENT (STREET AND CITY) 194 Eastlawn Ave Ste A St Robert, MO 65584		TIME OF INSPECTION 06:30:43

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>06/11/2022 06:30:45</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.7°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG208102</u>	EXP. DATE <u>03/22/2024</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIM. SN _____	SIM. NIST EXP DATE _____

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.	
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE	
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE	
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE	

TEST 1: 0.104	TEST 2: 0.104	TEST 3: 0.104
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:					
REFUSALS: 0	0-.04: 6	.05-.09: 0	.10-.14: 0	.15-.19: 1	OVER .19: 1

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER	
SIGNATURE 	PRINT FULL NAME TYSON E RUSSELL
TYPE II PERMIT NUMBER 220024	EXPIRATION DATE 01/24/2024
TELEPHONE NUMBER 573-336-4700	

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email

STANDARD CHANGE

St Robert Police Department
INTOX dmt: 500281

Date: 06/11/2022
Time: 06:27:12


OPERATOR NAME:
TYSON E RUSSELL
PERMIT NUMBER: 220024
EXPIRATION DATE: 01/24/2024

LOT #: AG208102
SUPPLIER: INTOXIMETERS
EXPIRATION: 03/22/2024
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.096

BLANK TEST	0.000	06:28
INTERNAL STANDARD	VERIFIED	06:28
EXTERNAL STANDARD	0.100	06:28
BLANK TEST	0.000	06:29

Average = 0.1000
Std Dev = 0.0000
Spread = 0.0000

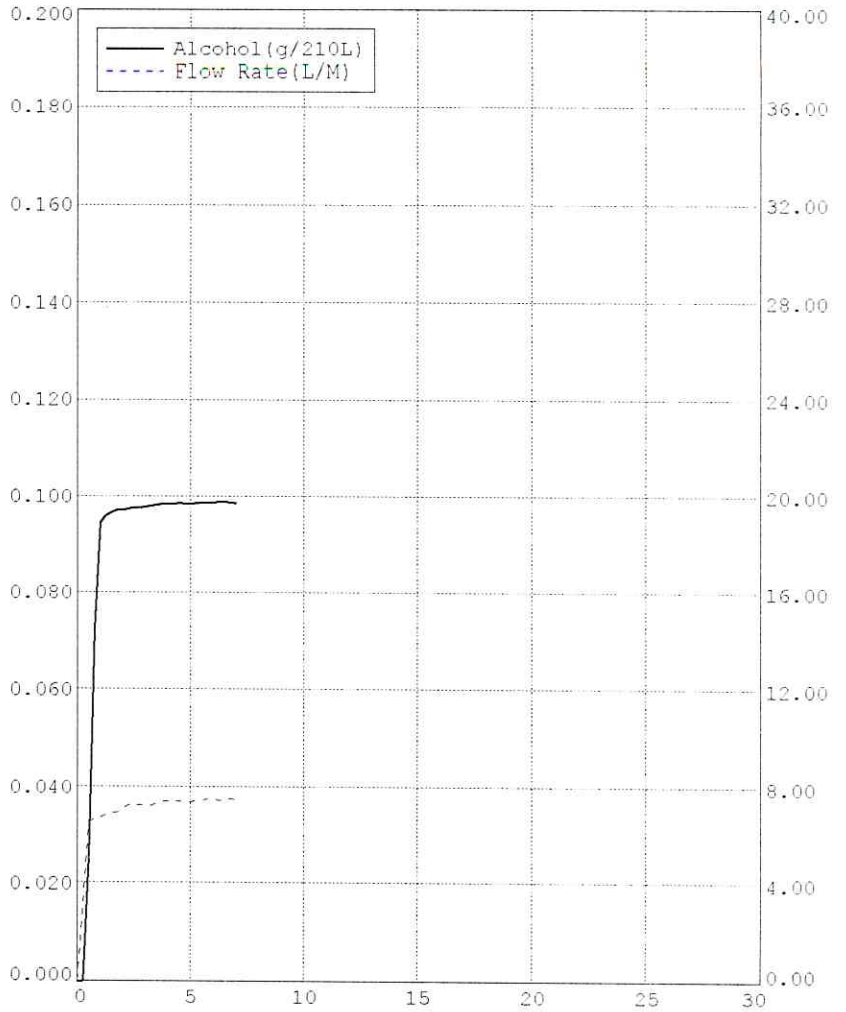

Handwritten signature and number 103



Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax: (314) 533-7328

Certificate of Analysis

Customer Name
Exclusive Supplier
 Intoximeters, Inc.
 2081 Craig Road
 St. Louis, Mo 63146

Test Date: 23-Mar-2022

Lot # AG208102 **Model** 108

Exp Date 22-Mar-2024	Cyl. Type 108	Component Ethanol Nitrogen	Certified Concentration 0.100 ± 2% BrAC (260 ppm)
--------------------------------	-------------------------	---	---

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010562	104.2 ppm
EB0010561	103.7 ppm	EB0010579	52.94 ppm
EB0010681	52.22 ppm		

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CC727481	800.0 ppm	CC727493	390.0 ppm
CC727496	253.0 ppm	CC727498	150.0 ppm

Analytical Method: NDIR

Approved for Release: 
 Rod Marsala

ISO 17025:2017 A2LA accredited. Certificate Number 3082.06
ISO 17034:2016 A2LA accredited. Certificate Number 3082.07

