



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM

**RECEIVED**  
By Tracy Crews at 11:32 am, Jul 28, 2024

**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500252	NAME OF AGENCY Cameron Police Department	DATE OF INSPECTION 07/27/2024
LOCATION OF INSTRUMENT (STREET AND CITY) 101 North Chestnut, Cameron, Missouri 64429		TIME OF INSPECTION 01:32:14

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

DATE AND TIME <u>07/27/2024 01:32:16</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.9°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

**BREATH ANALYZER ACCURACY STANDARDS**

SIMULATOR STANDARD       COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS      LOT # AG310901      EXP. DATE 04/19/2025

SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_      SIM. SN \_\_\_\_\_      SIM. NIST EXP DATE \_\_\_\_\_

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.080	TEST 2: 0.080	TEST 3: 0.080
---------------	---------------	---------------

**PERFORM R.F.I. TEST**

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 16	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	-----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME JAMES C PROCTOR	
TYPE II PERMIT NUMBER 230062	EXPIRATION DATE 04/02/2025	TELEPHONE NUMBER 816-632-6521

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email



Airgas USA LLC (LAB)  
 3500 Bernard Street  
 St. Louis, Mo. 63103  
 Ph: (314) 533-3100  
 Fax: (314) 533-7328

## Certificate of Analysis

Customer Name  
 Exclusive Supplier  
 Intoximeters, Inc.

Test Date: 20-Apr-2023

~~2081 Craig Road~~  
 St. Louis, Mo 63145

Lot # AG310901 Model 108

Exp Date	Cyl. Type	Component	Certified Concentration
19-Apr-2025	108	Ethanol Nitrogen	0.080 ± 0.002 BrAC (ZDB ppm)


Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	391.8 ppm	EB0010603	352.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010562	104.2 ppm
EB0010561	103.7 ppm	EB0010579	52.94 ppm
EB0010681	52.22 ppm		

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CCTZ7481	800.0 ppm	CCTZ7493	390.0 ppm
CCTZ7496	253.0 ppm	CCTZ7498	150.0 ppm

Analytical Method: NDIR

Digitally signed by Quality Control  
 Reason: Dry gas standard certification of analysis  
 Location: Airgas USA, LLC (Lab)  
 Date: 04.20.2023 14:28

Approved for Release:   
 Rod Marsala

ISO 17025:2017 A2LA accredited. Certificate Number 3082.06  
 ISO 17034:2016 A2LA accredited. Certificate Number 3082.07



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 101 North Chestnut, Cameron, Missouri	INSTRUMENT SERIAL NUMBER 500252	DATE OF TEST 07/27/2024	TIME OBSERVATION PERIOD STARTED 01:15	TIME OF TEST 01:41:16
SUBJECT NAME MONTHLY TEST			DATE OF BIRTH 01/01/2020	
SUBJECT DRIVER'S LICENSE NUMBER MO07272024			STATE MO	
ARRESTING OFFICER JAMES C PROCTOR		ARRESTING OFFICER ID 107		
OPERATOR JAMES C PROCTOR		OPERATOR PERMIT 230062	PERMIT EXP DATE 04/02/2025	
OBSERVER JAMES C PROCTOR		OBSERVER PERMIT 230062	PERMIT EXP DATE 04/02/2025	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JAMES C PROCTOR. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	01:42
INTERNAL STANDARD	VERIFIED	01:42
SUBJECT SAMPLE (Vol=2.10L)	0.000	01:42
BLANK TEST	0.000	01:43

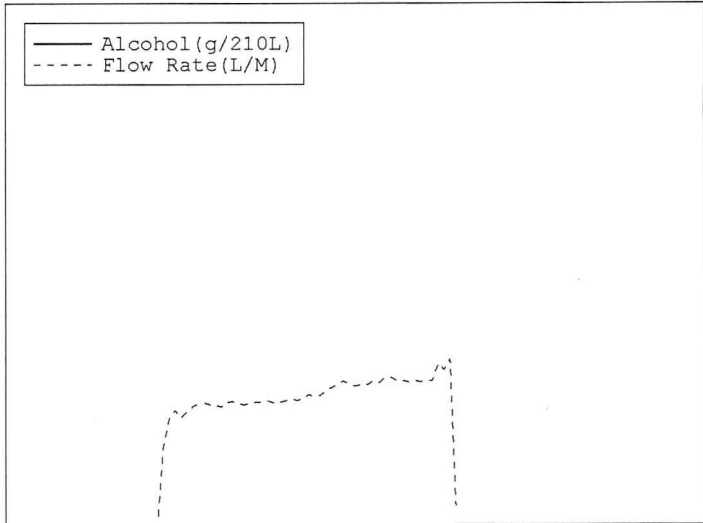

COMMENTS

CERTIFICATION BY OPERATOR

BAC  
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.


SIGNATURE OF OPERATOR

DATE  
07/27/2024

WITNESS (IF ANY)

DATE  
07/27/2024





STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM



PERMIT  
 TYPE II

**JAMES C. PROCTOR**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 572.020 through 572.041, RSMo and 306.111 through 306.116 RSMo.

DATE: 4/2/2023

NUMBER: 230062

EXPIRES: 4/2/2025


*[Signature]*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*[Signature]*

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LS&H 16711B



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator: PROCTOR, JAMES  
 Permit No: 230062  
 Date Issued: 4/2/2023 Date Expires: 4/2/2025

